

Holder Blocker Selection Guide

Important: Be sure to include Shipping Address with order.

175 Series: (3/4" tape width)

Select Holder Blocker Using Kvp-MAS Chart below.
Specify quantity in box next to style and check appropriate density (density is in parenthesis):

QUANTITY

175A

DOCTOR OR COMPANY NAME
ADDRESS, CITY, STATE

- (I) White
 (II) Green
 (III) Yellow
 (IV) Red

176A

DOCTOR OR COMPANY NAME R
ADDRESS, CITY, STATE L

- (I) White
 (II) Green
 (III) Yellow
 (IV) Red

177A

DOCTOR OR COMPANY NAME A
ADDRESS, CITY, STATE M L P

- (I) White
 (II) Green
 (III) Yellow
 (IV) Red

178A

DOCTOR OR COMPANY NAME LF RF
ADDRESS, CITY, STATE LH RH

- (I) White
 (II) Green
 (III) Yellow
 (IV) Red

138 Series: (3/8" tape width)

Select Holder Blocker Using Kvp-MAS Chart below.
Specify quantity in box next to style and check appropriate density (density is in parenthesis):

QUANTITY

138A
Standard

DOCTOR OR COMPANY NAME
ADDRESS, CITY, STATE

- (I) White
 (II) Green

138B
Curved

DOCTOR OR COMPANY NAME
ADDRESS, CITY, STATE

- (I) White
 (II) Green

138C
Flexible

DOCTOR OR COMPANY NAME
ADDRESS, CITY, STATE

- NOTE:**
138C Flexible
comes in one
density Only
Blue only

139A

DOCTOR OR COMPANY NAME R
ADDRESS, CITY, STATE L

- (I) White
 (II) Green

Imprint: (PLEASE PRINT CLEARLY) **MAXIMUM 26 CHARACTERS INCLUDING SPACES**

TOP LINE

--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--

BOTTOM LINE

--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--	--

DEALER:

DEALER NAME _____ ACCT.# _____

ADDRESS _____

CITY _____ STATE _____ ZIP _____

PHONE (____) _____

SHIP TO:

NAME _____


ADDRESS _____

CITY _____ STATE/ PROVINCE _____ ZIP _____

COUNTRY _____ PHONE (____) _____

ATTN: _____

Kvp-MAS CHART
Color Represents Density Level

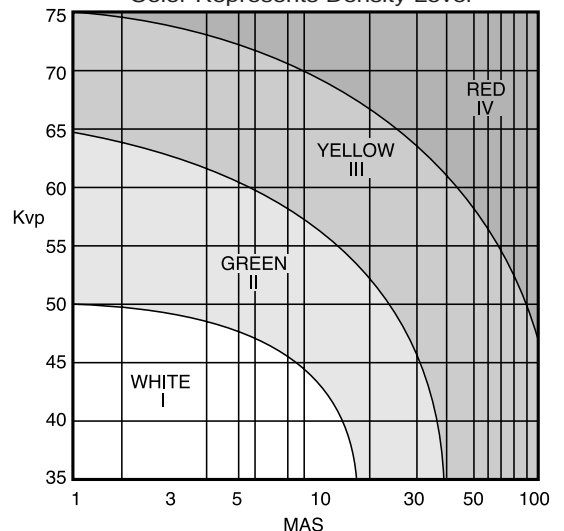

Holder Blocker User Guide

Here's how to select the right X-Rite holder blocker for your needs:

- Identify the Kvp and MAS used for your X-ray technique.
- Refer to the chart and select the appropriate holder blocker required.
- If desired, each holder blocker can be customized with the physician's name or the clinic's name as well as the clinic's location (city and state). Limit is 26 characters on both the top and bottom lines.

When an exposure is made with the holder blocker in place this customized information is automatically recorded on the film.

Holder Blockers for Specific Systems:

Dental:

CEPHLAMETRIC - 138A-Flat-(II) Green
PANORAMIC - 138B-Curved-(I) White
BAG CASSETTE - 138C - Flexible - Blue Only

General and Veterinary:

WHITE - Dental, Feet, Small Animals and Bones
GREEN - Arms, Medium Animals
YELLOW - Large Animals, Back and Chest
RED - Cows and Horses, Some Chiropractic Applications


How to Use X-Rite Marking Tape



Cut the tape to the desired length... or use pre-cut 3" strips.



Using a ballpoint pen, press firmly and print the patient's name on the marking tape.



Remove the paper backing by folding slightly to split the two pieces.



Affix the tape to the correct holder blocker with the tape's black area centered down the blocker's length. Use the overhanging tape to affix the label to the tube side of a cassette.

(Caution: do not place the tape and holder blocker in an area where a cassette has an identification window. The lead behind the intensifying screen does not allow for proper tape identification.)



Place the cassette and make the exposure.



Note:

If the tape and holder blocker are too light to identify, select the next lower holder blocker on the chart; if the tape and holder blocker are too dark, select the next higher one.

When using a KVP higher than 80, the holder blocker and tape can be located in an area behind tissue so that the patient will filter the excess radiation. A lower numbered holder blocker may have to be used.

X-Rite

X-Rite, Incorporated - World Headquarters

3100 44th Street, SW • Grandville, Michigan 49418 USA • 616 534-7663

L1-014 (3/98)